

FIG. 1 (Prior Art)

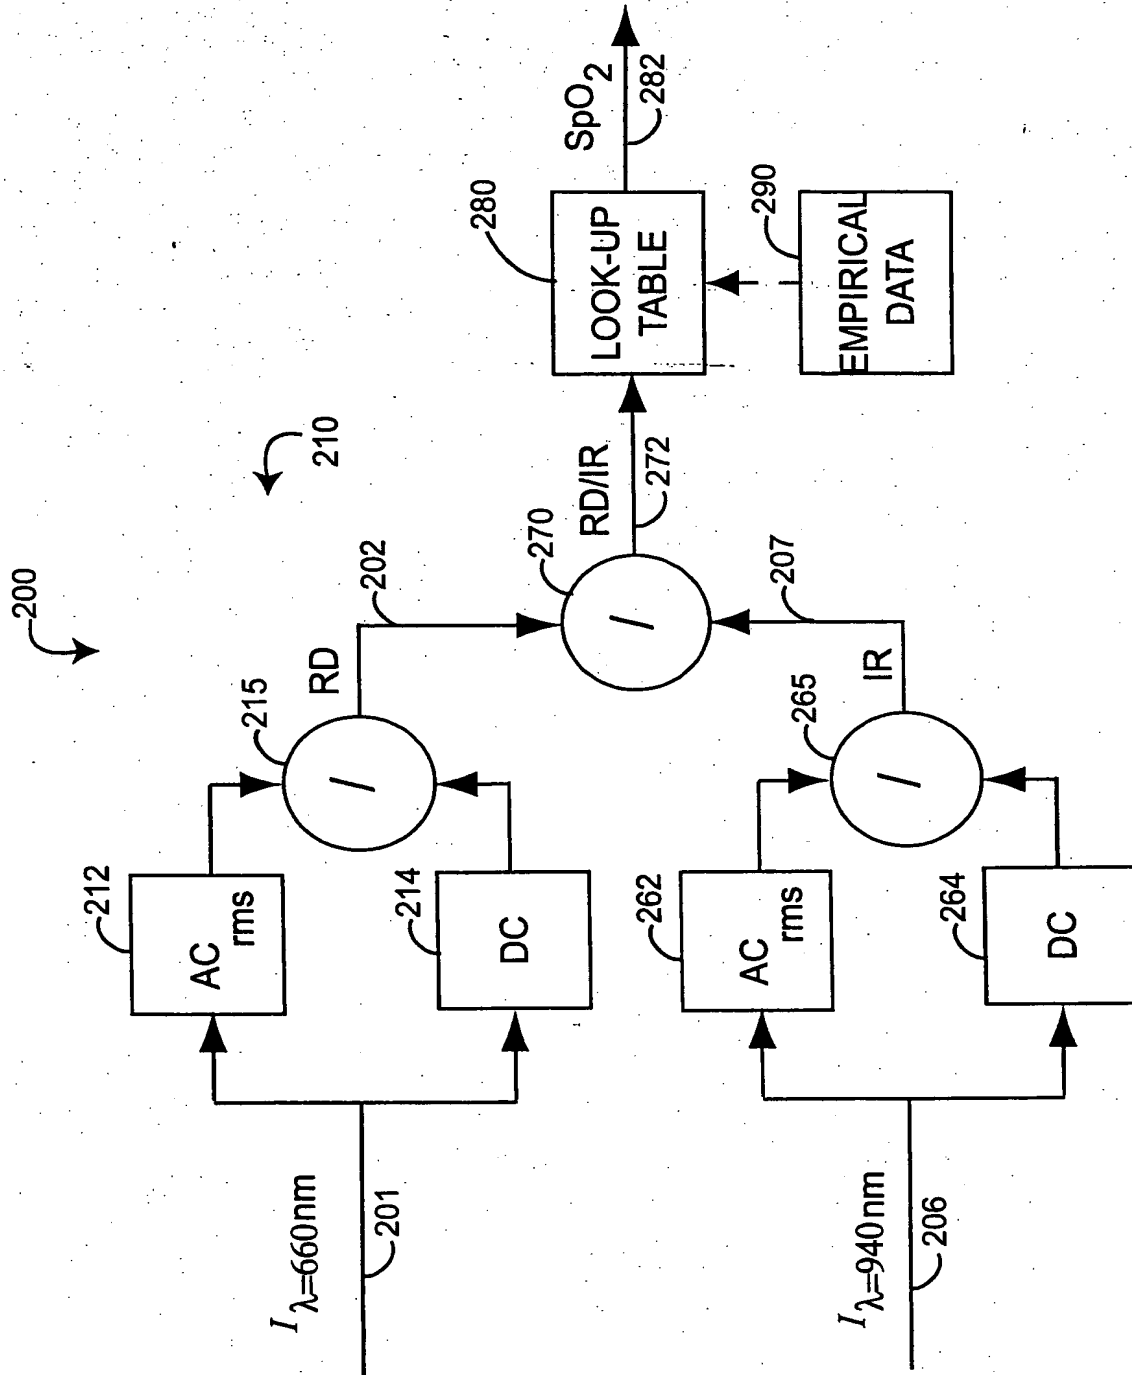


FIG. 2 (Prior Art)

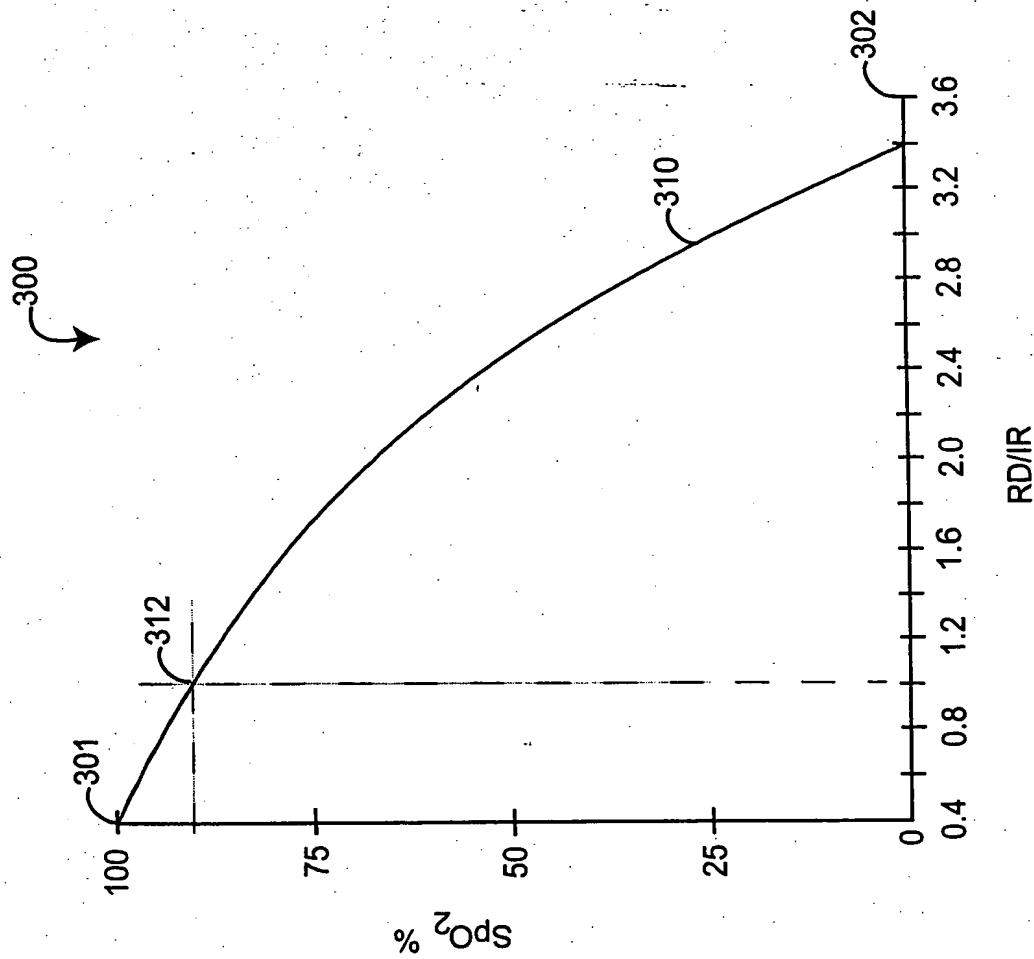


FIG. 3 (Prior Art)

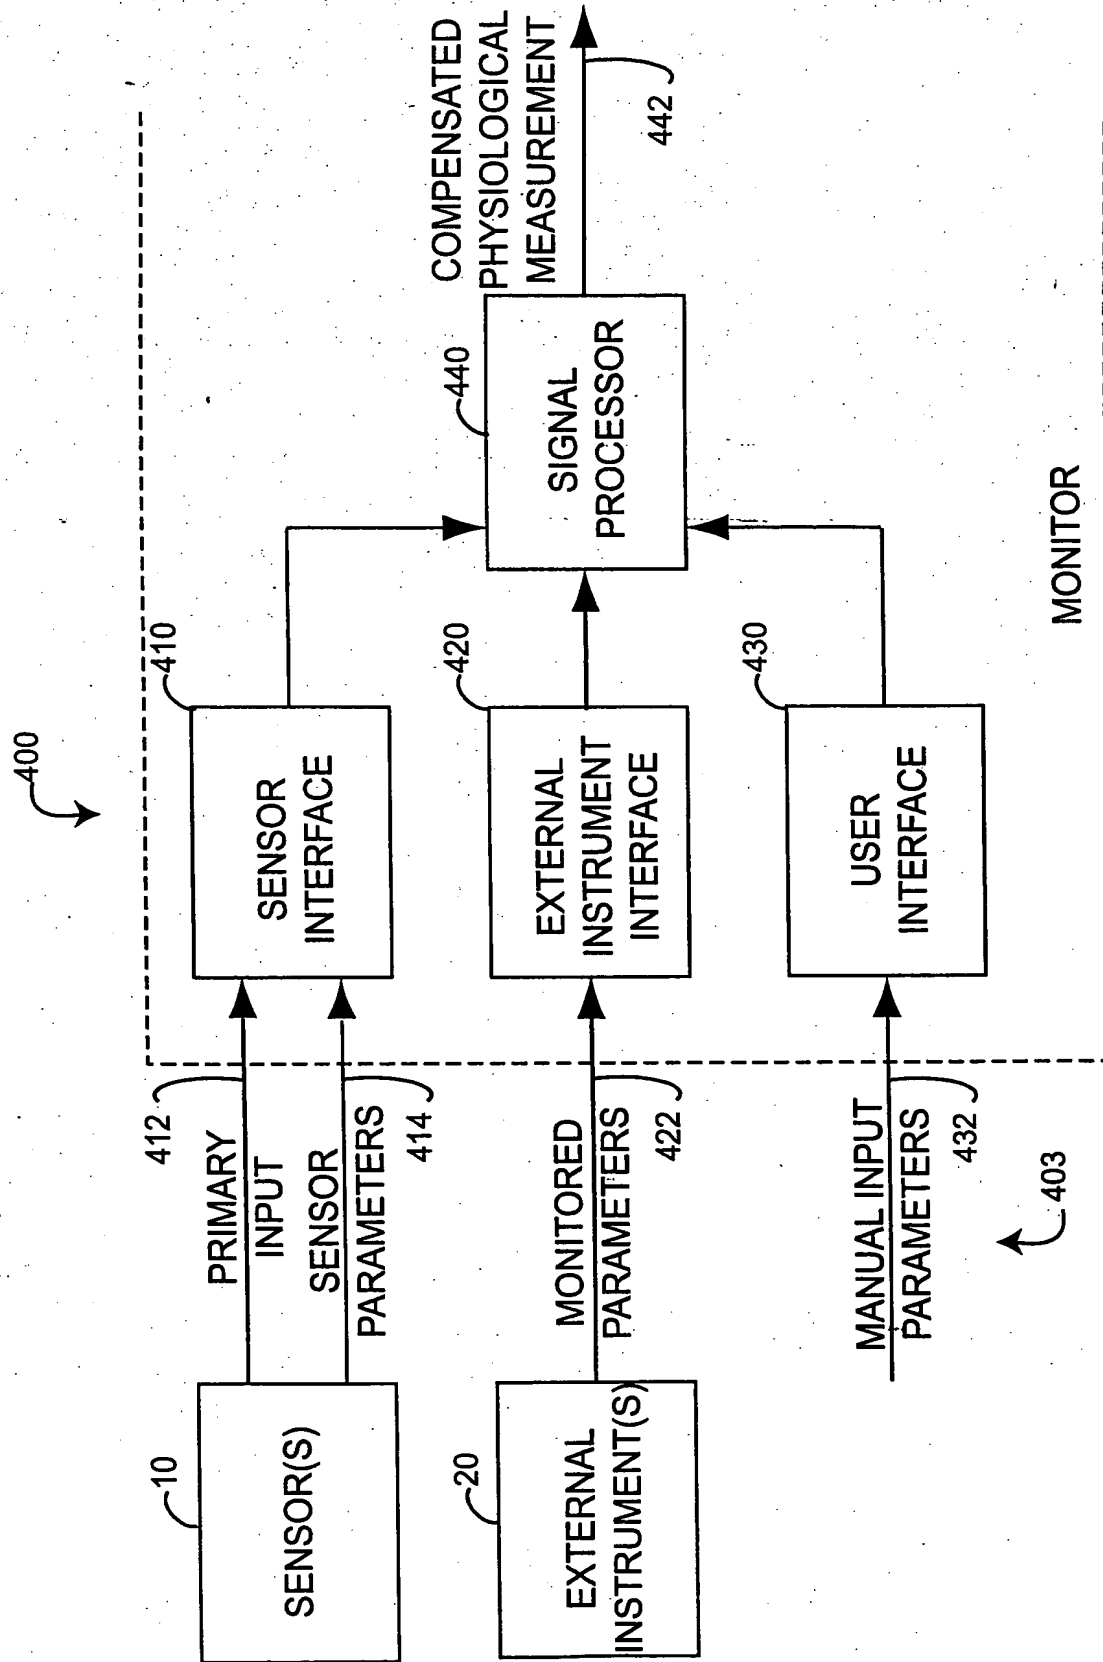


FIG. 4

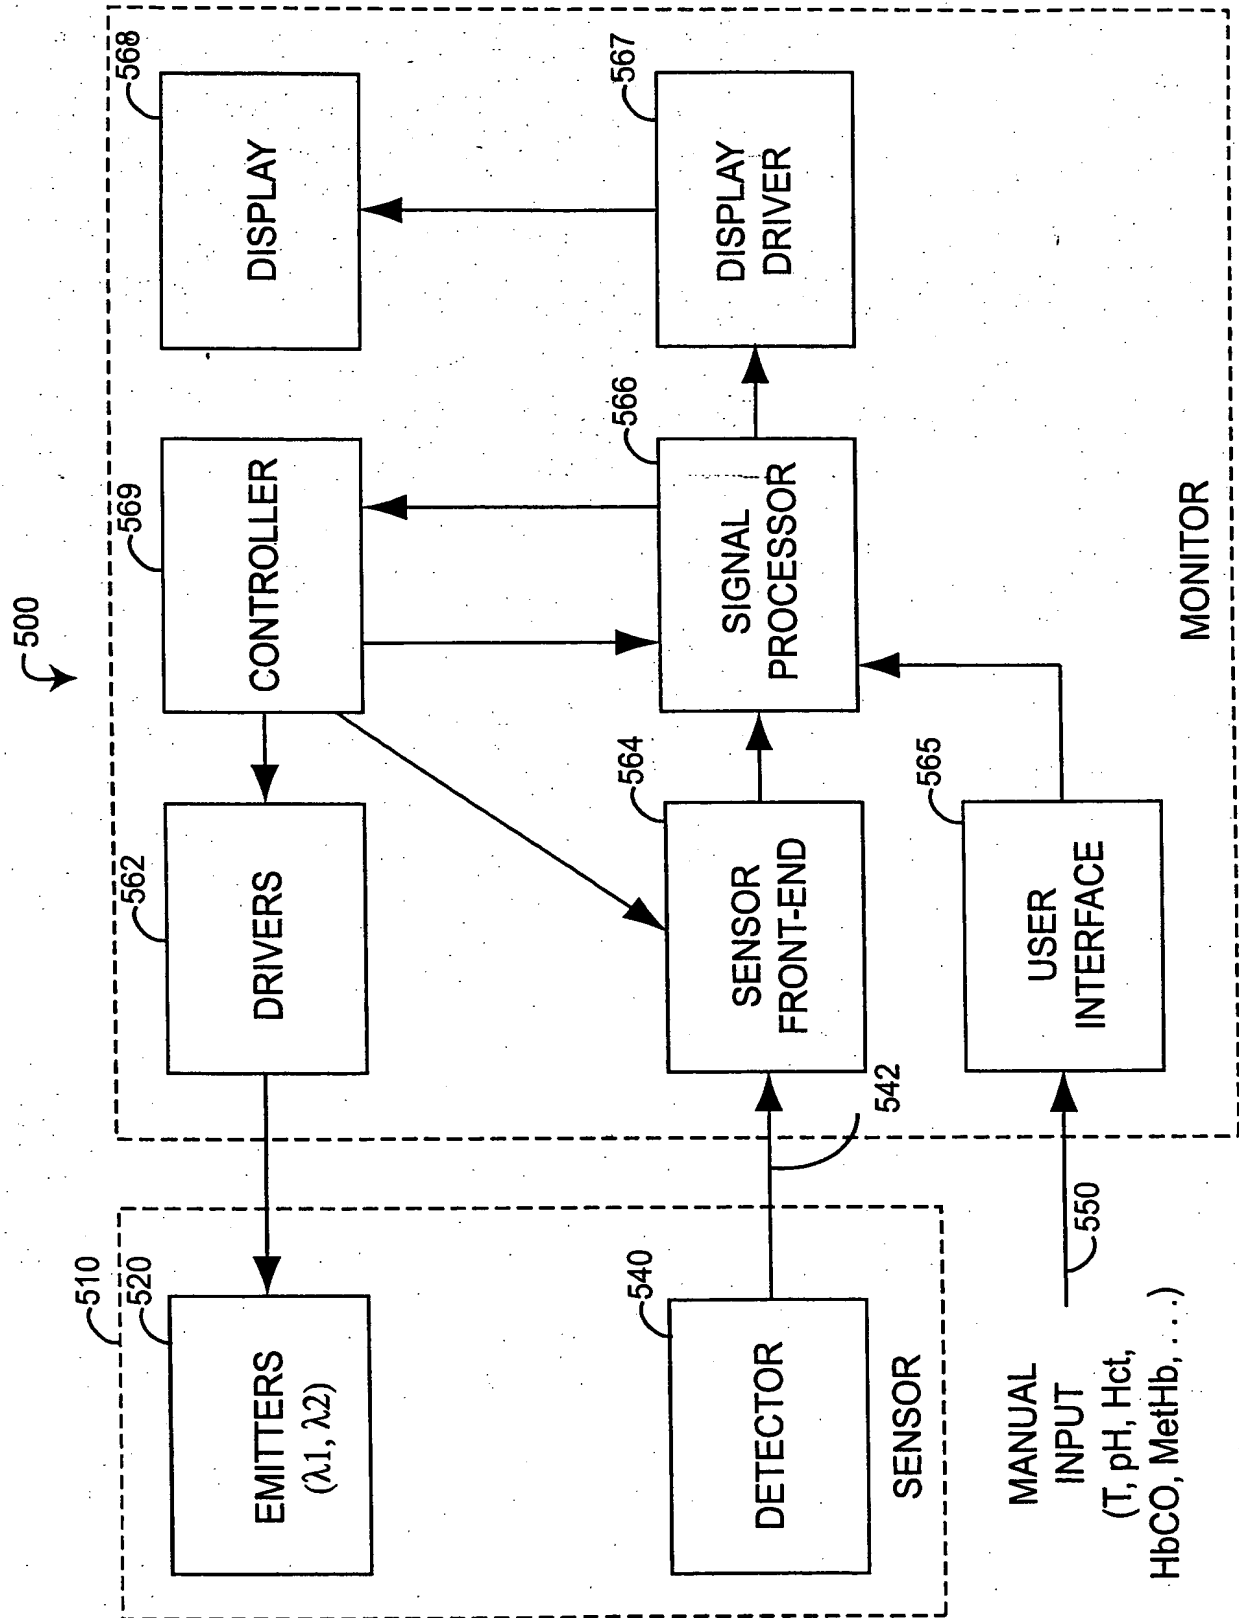


FIG. 5



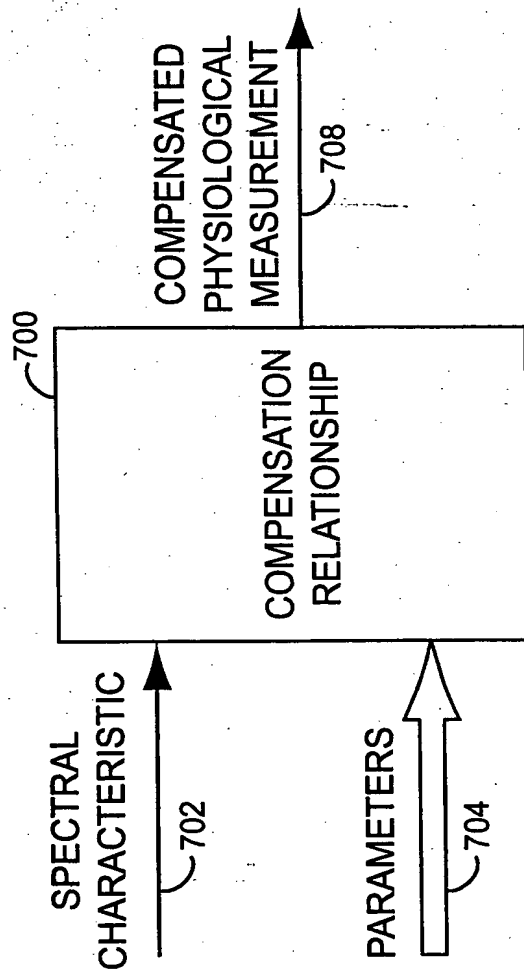


FIG. 7

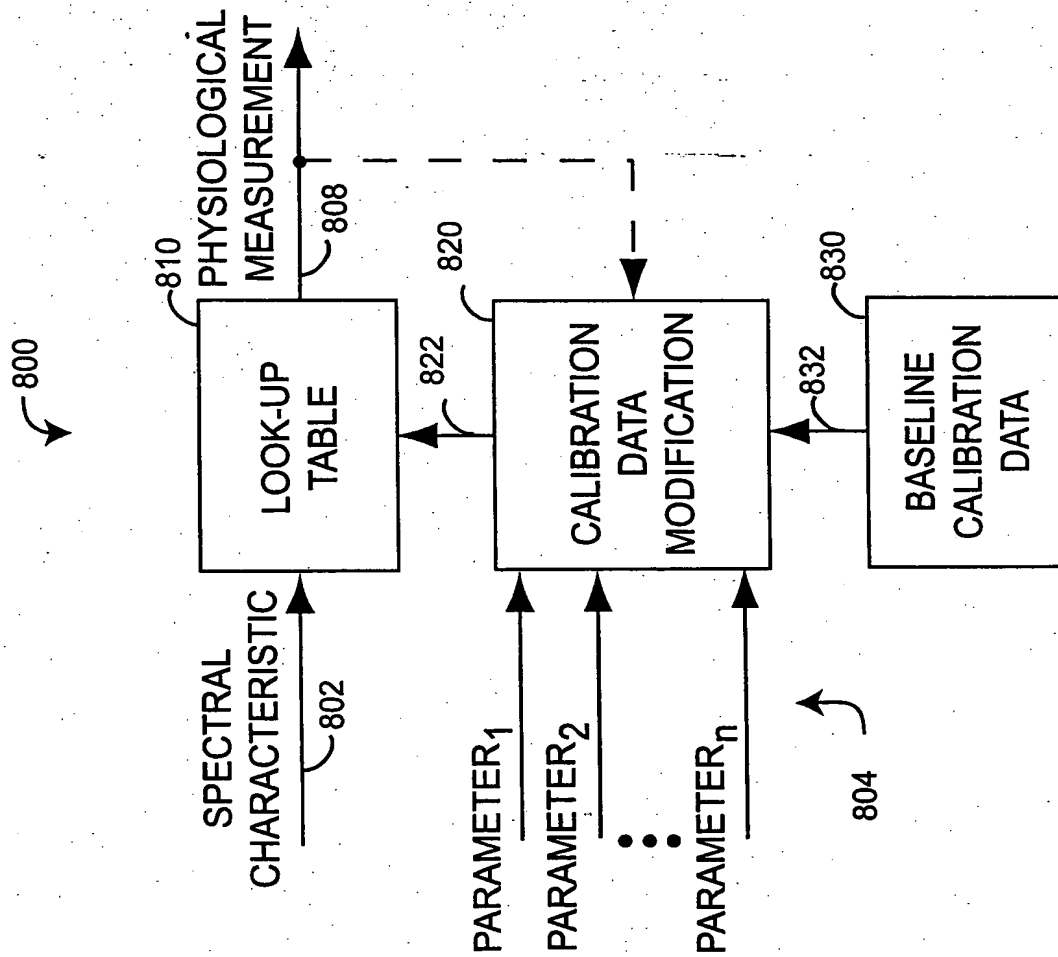


FIG. 8A



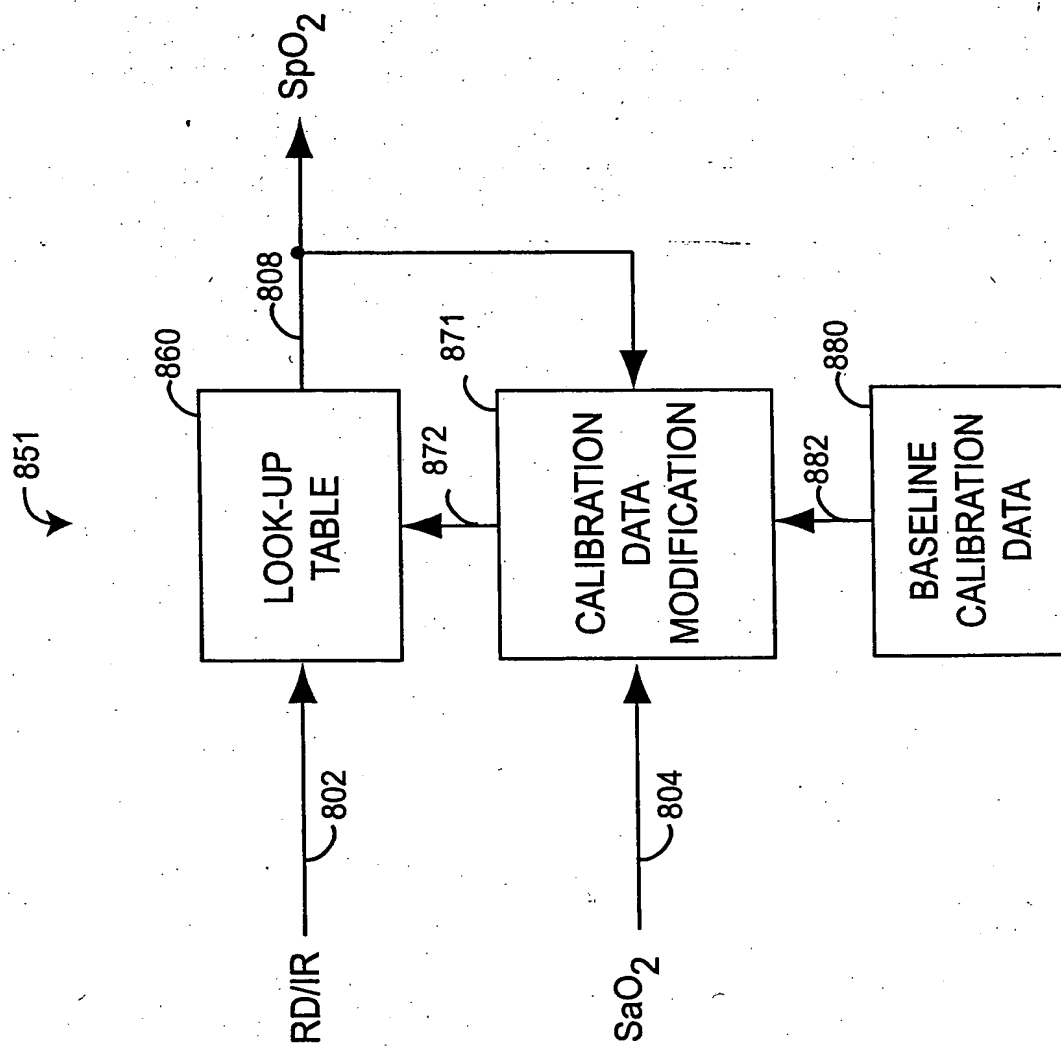


FIG. 8B

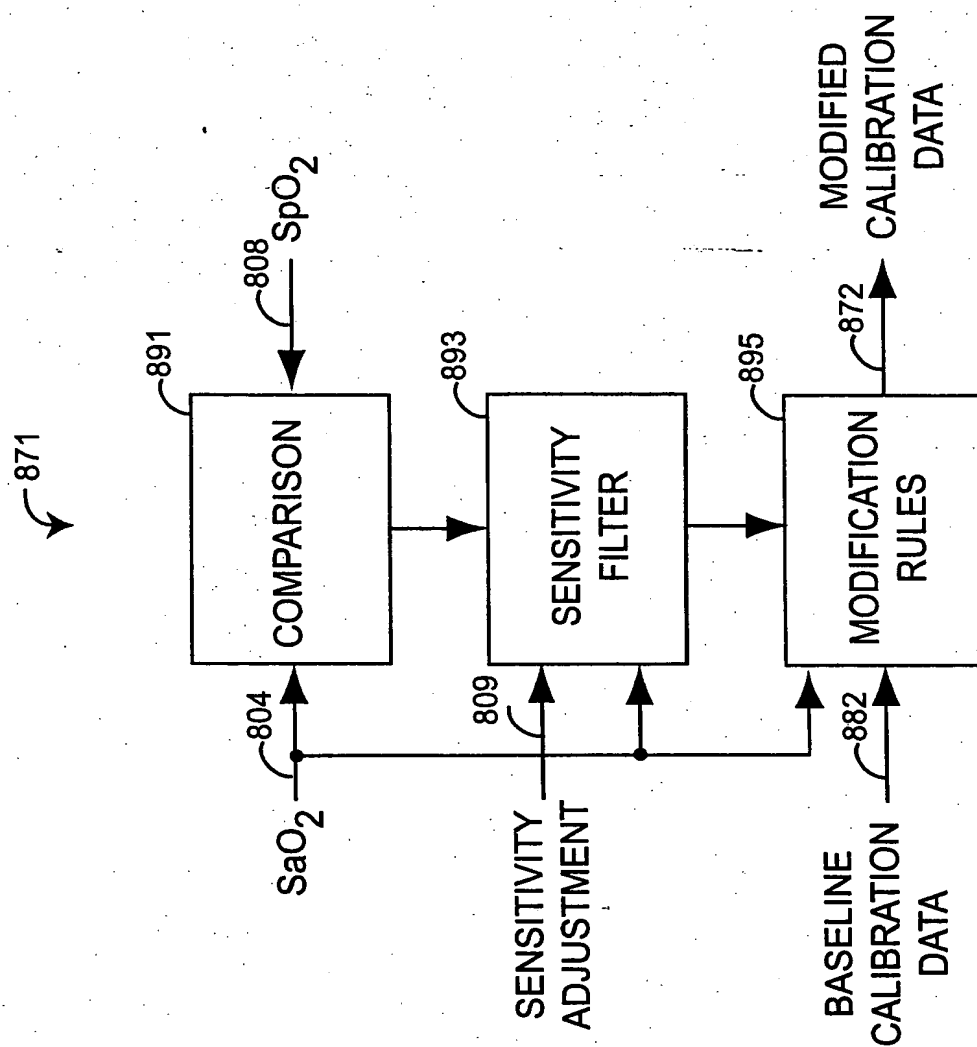


FIG. 8C

PARAMETER COMPENSATED PHYSIOLOGICAL MONITOR

Massi E. Kiani, et al.

Appl. No.: Unknown

Atty Docket: MASIMO.377A

11 / 19

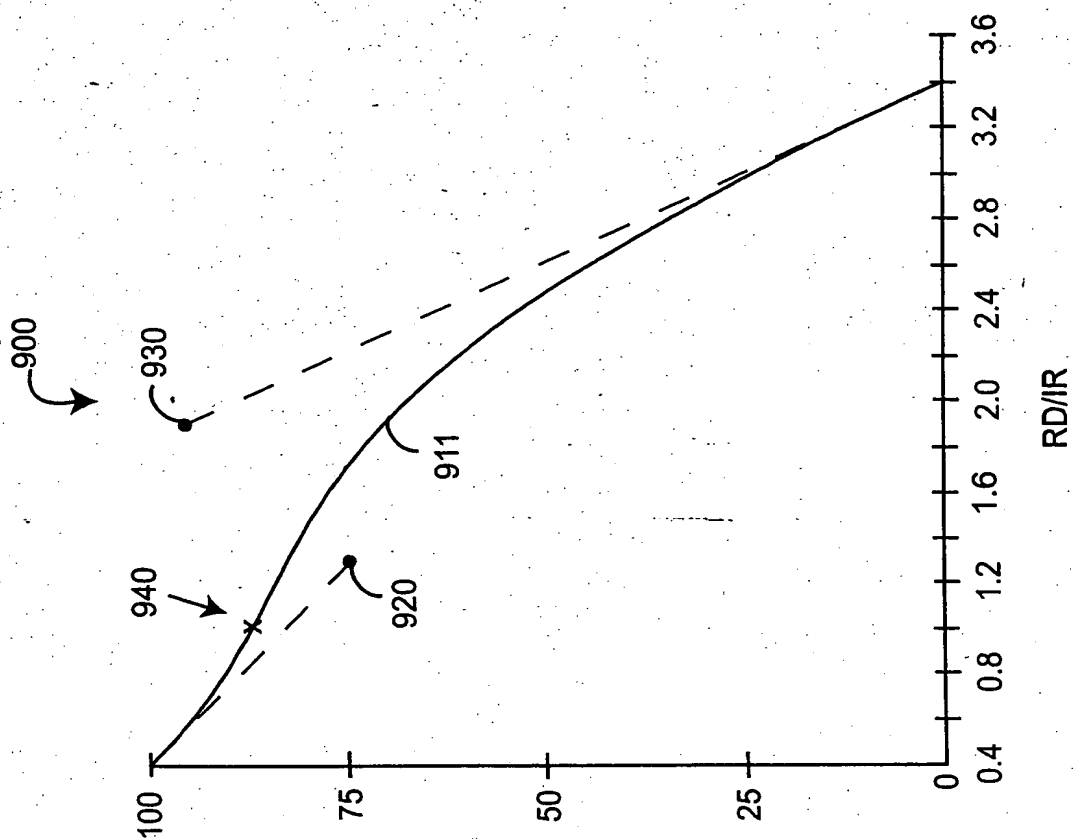


FIG. 9B

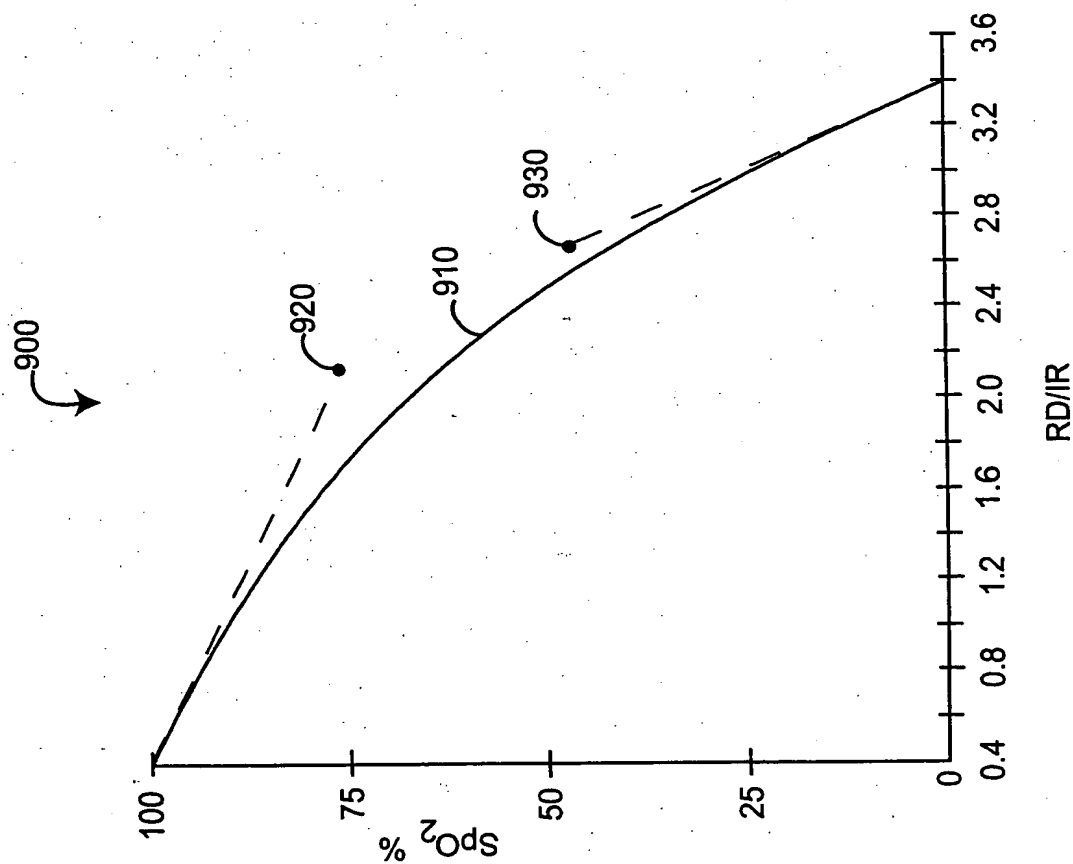


FIG. 9A

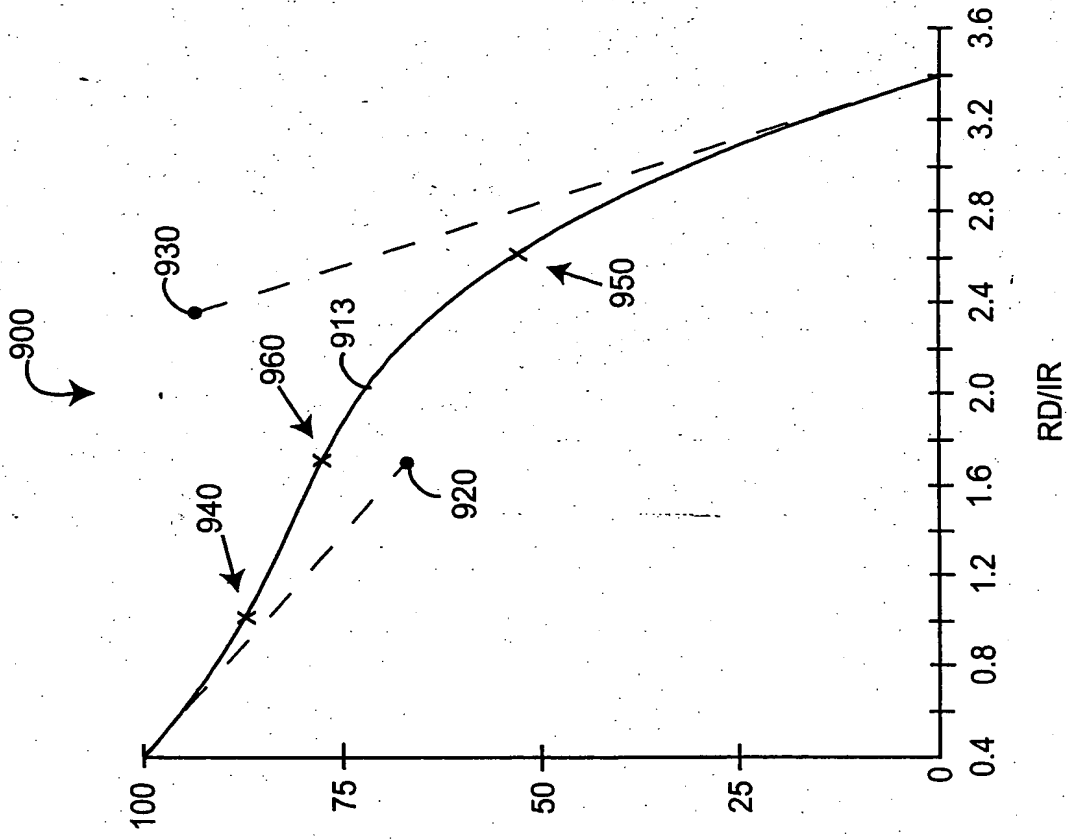


FIG. 9D

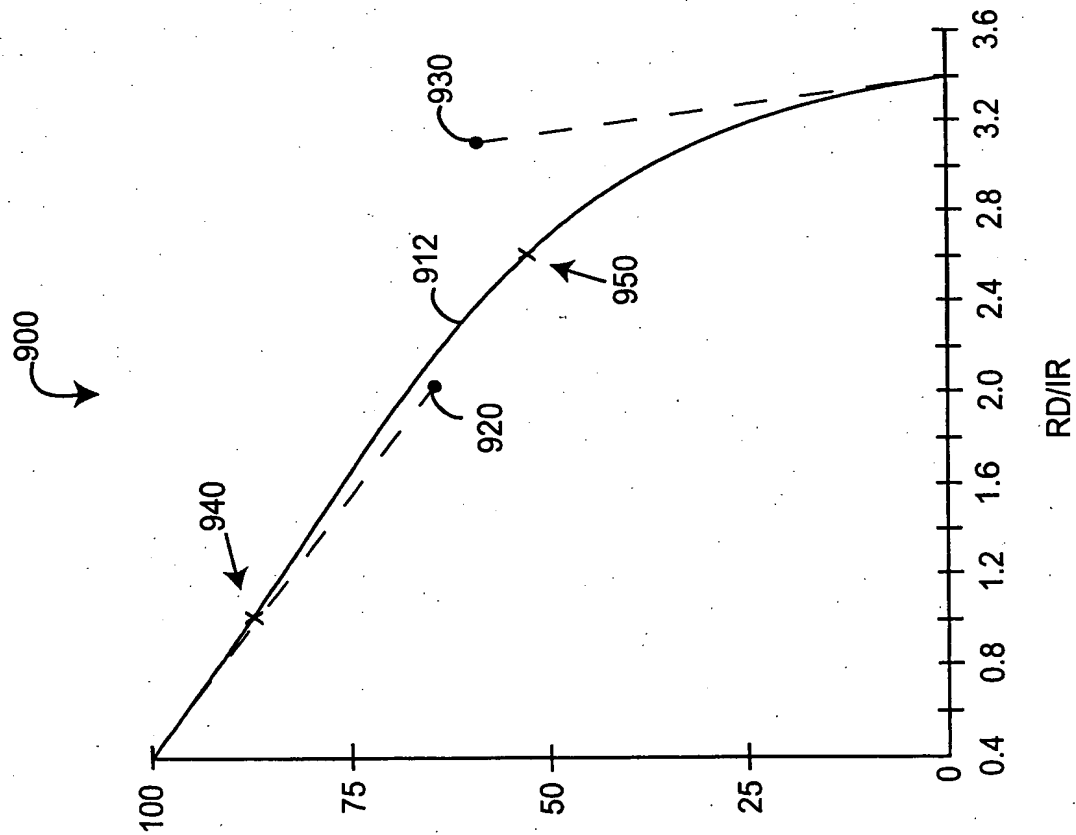


FIG. 9C

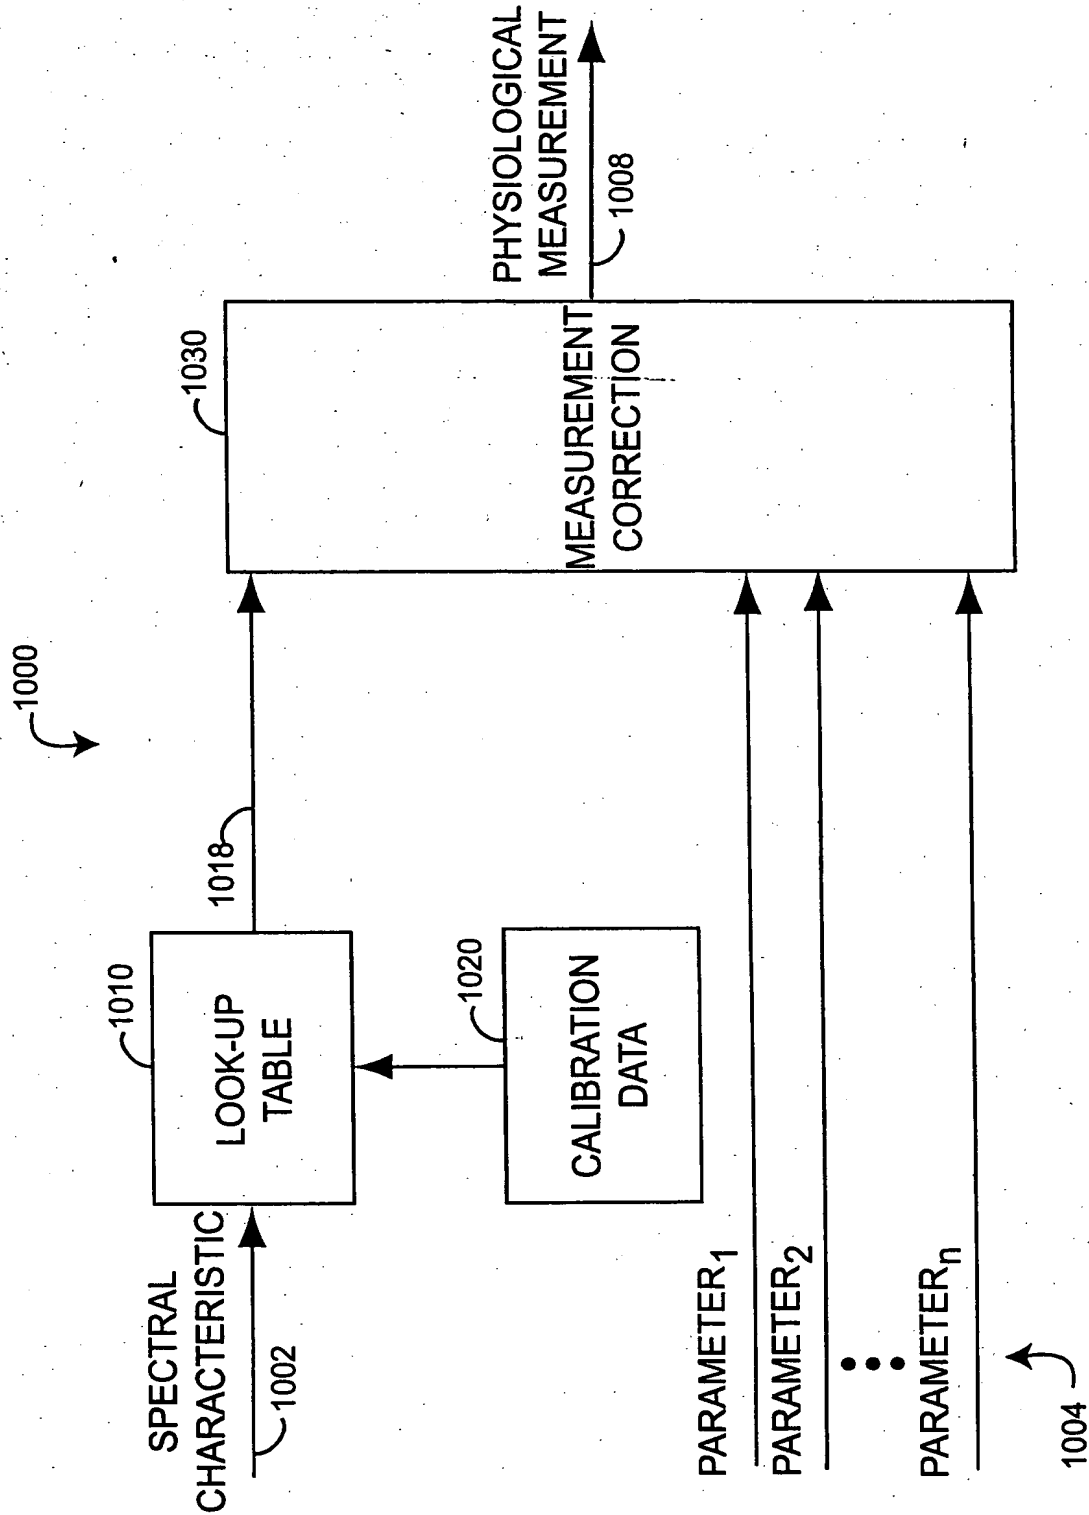


FIG. 10A

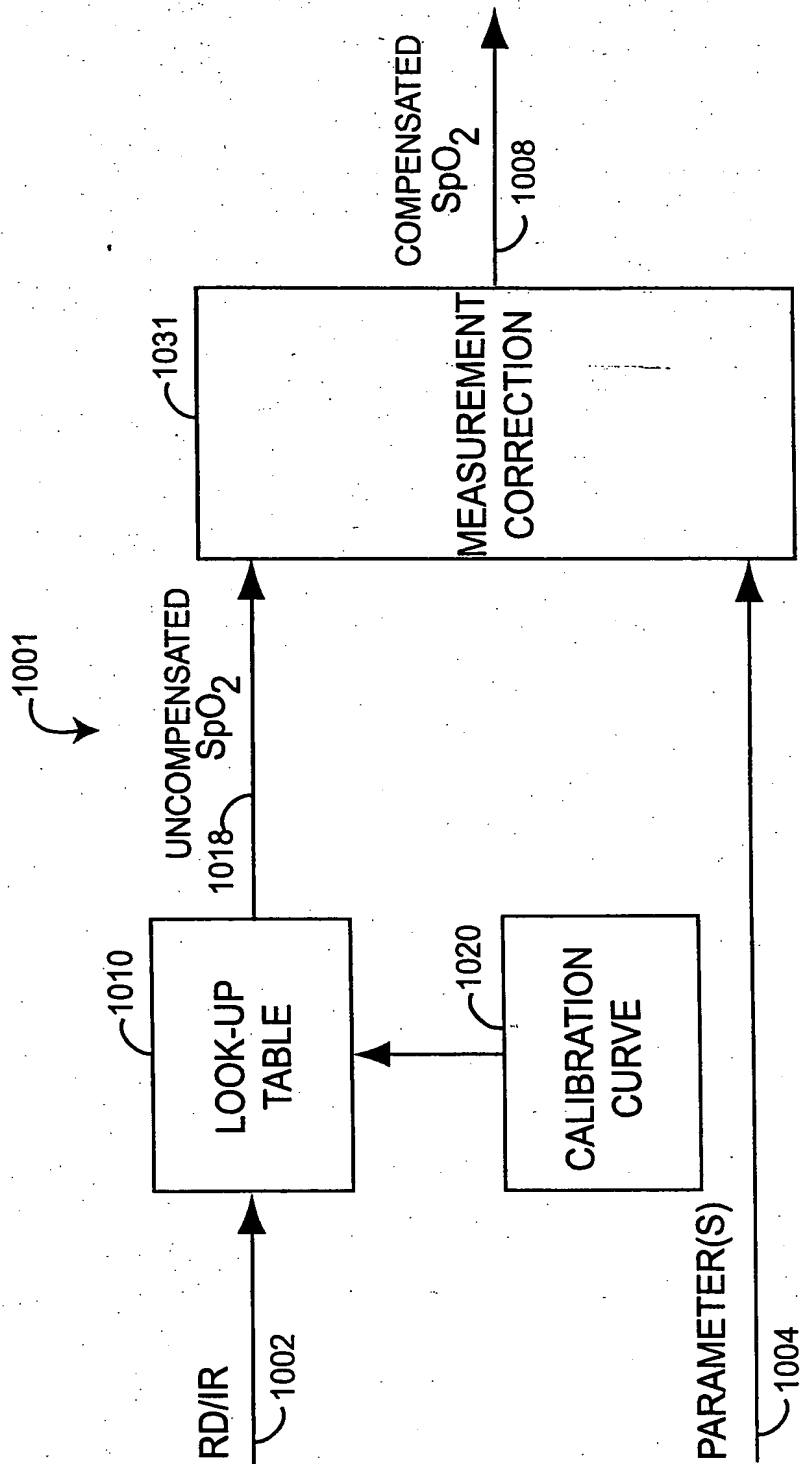


FIG. 10B

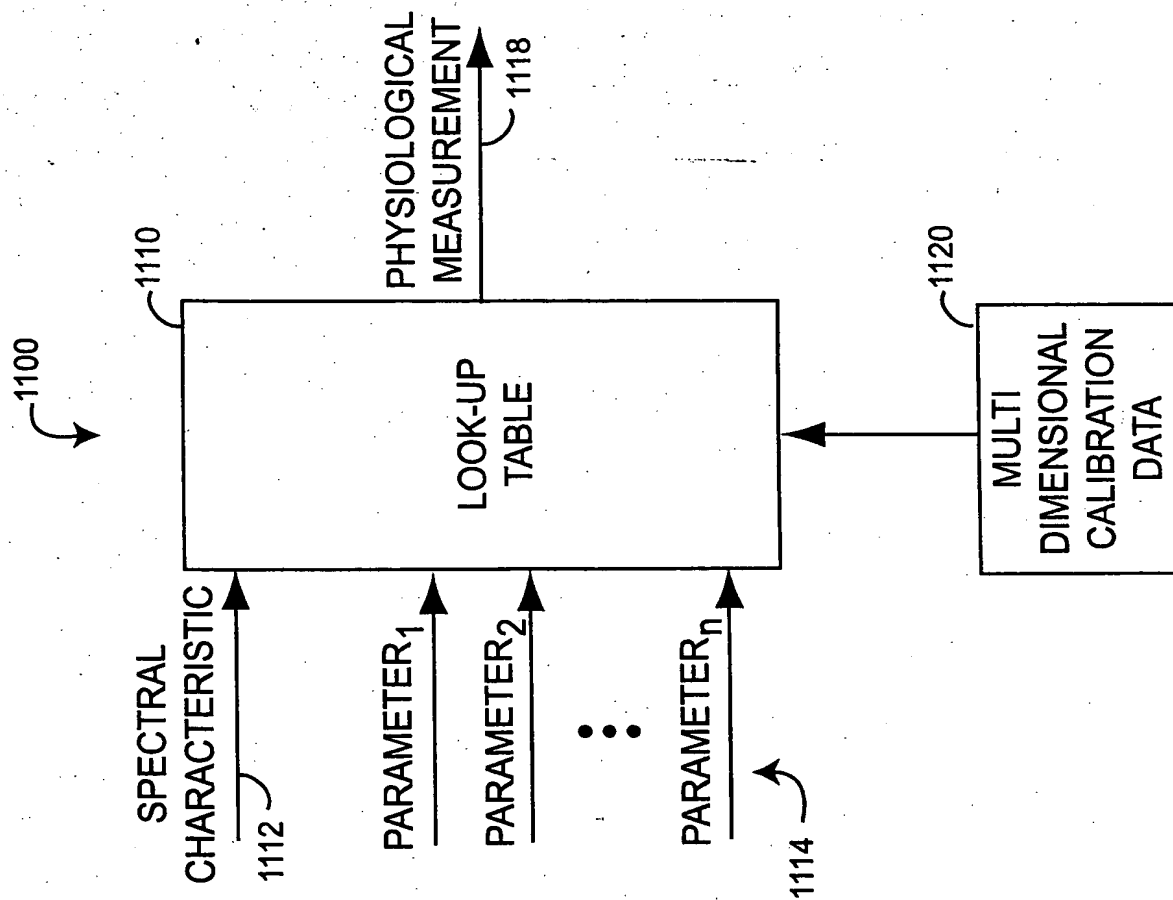


FIG. 11

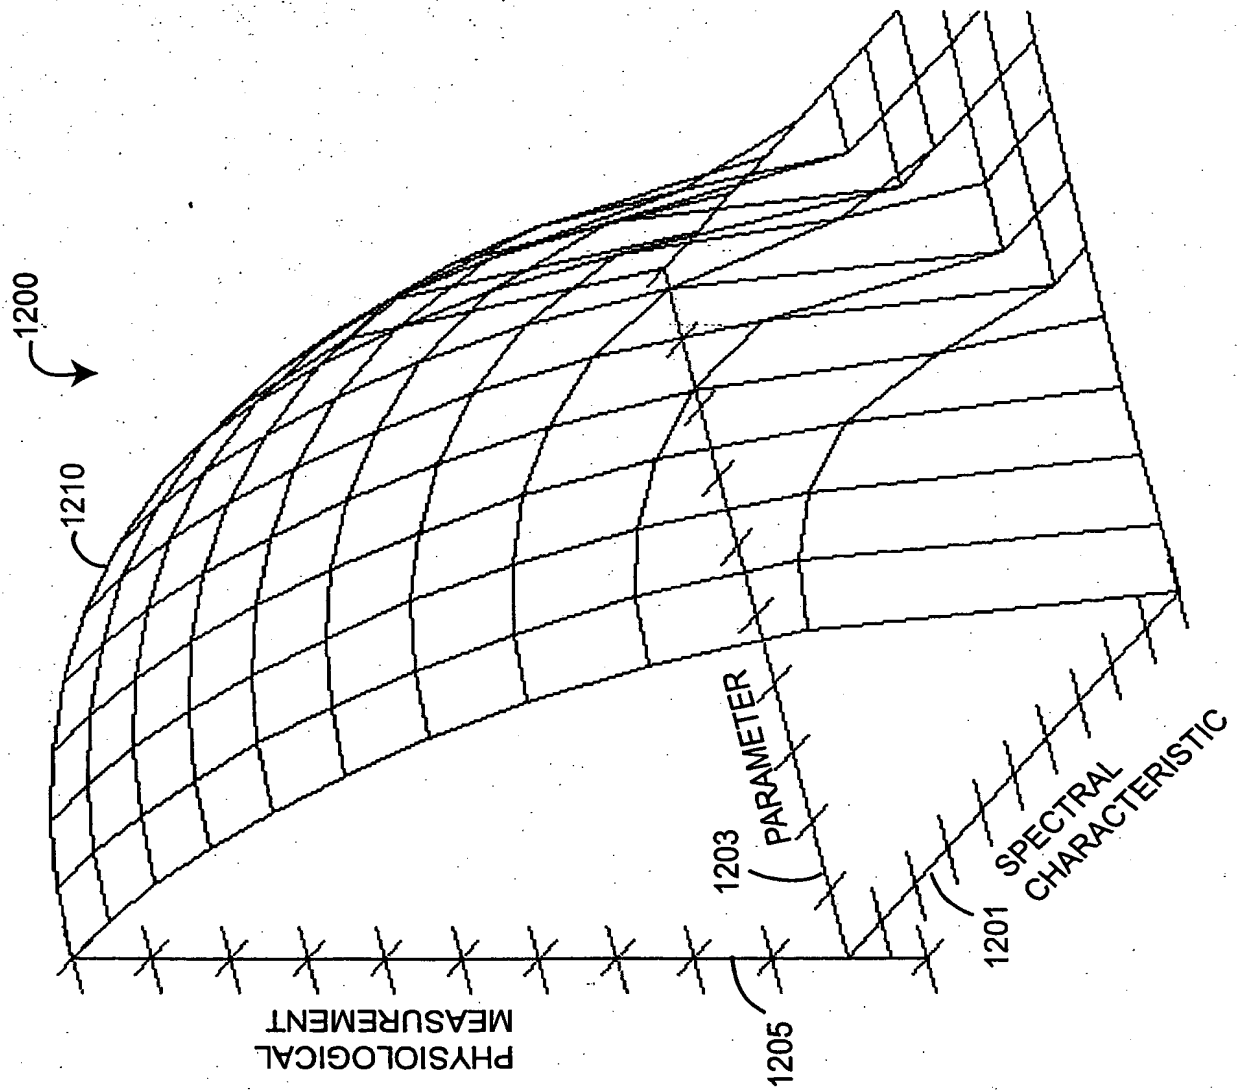


FIG. 12



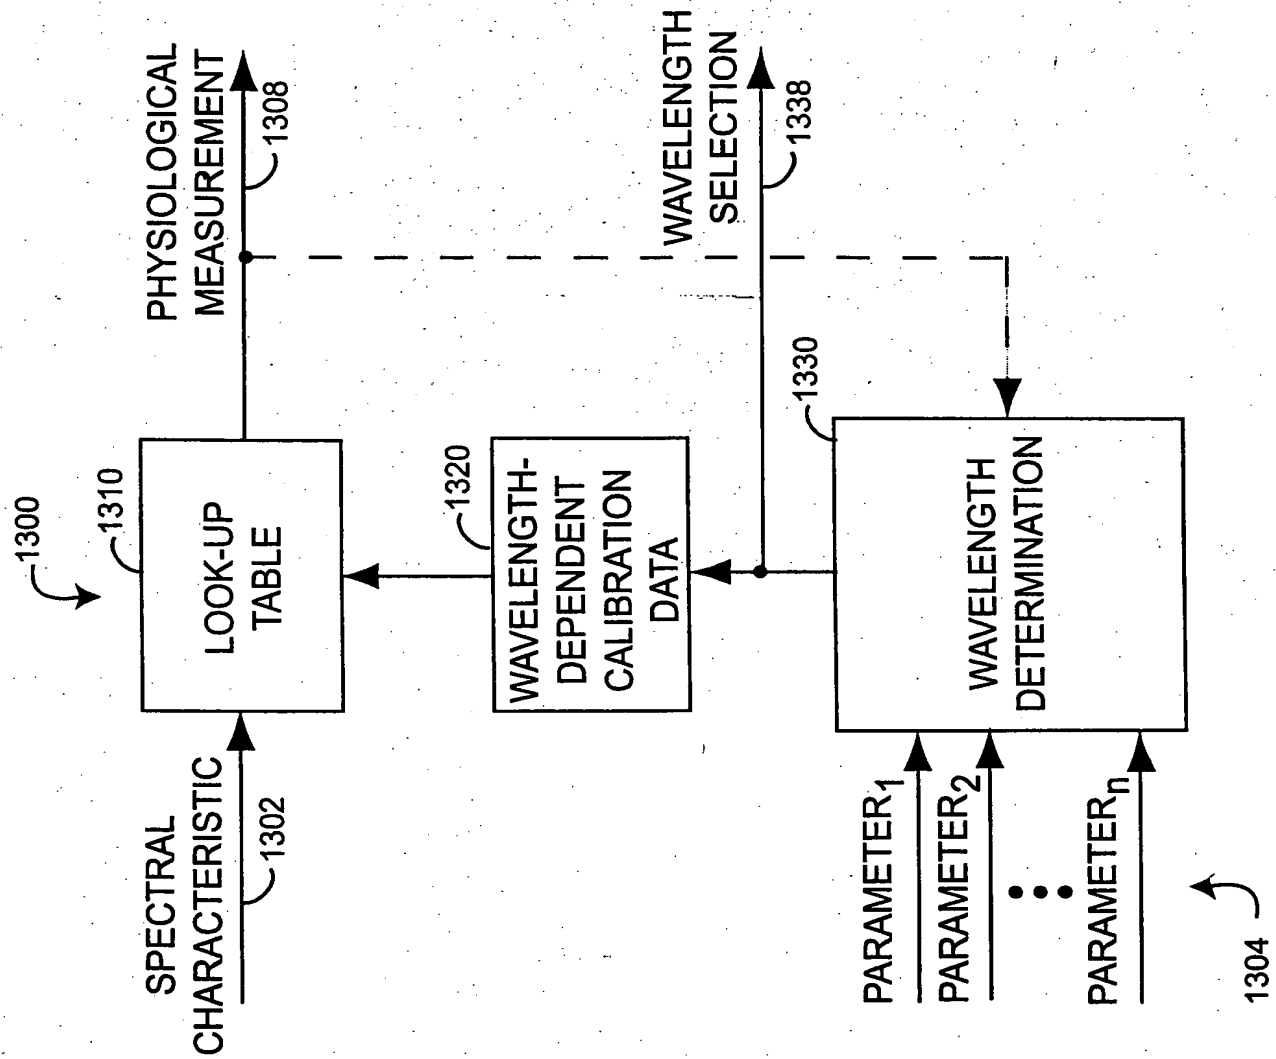


FIG. 13A

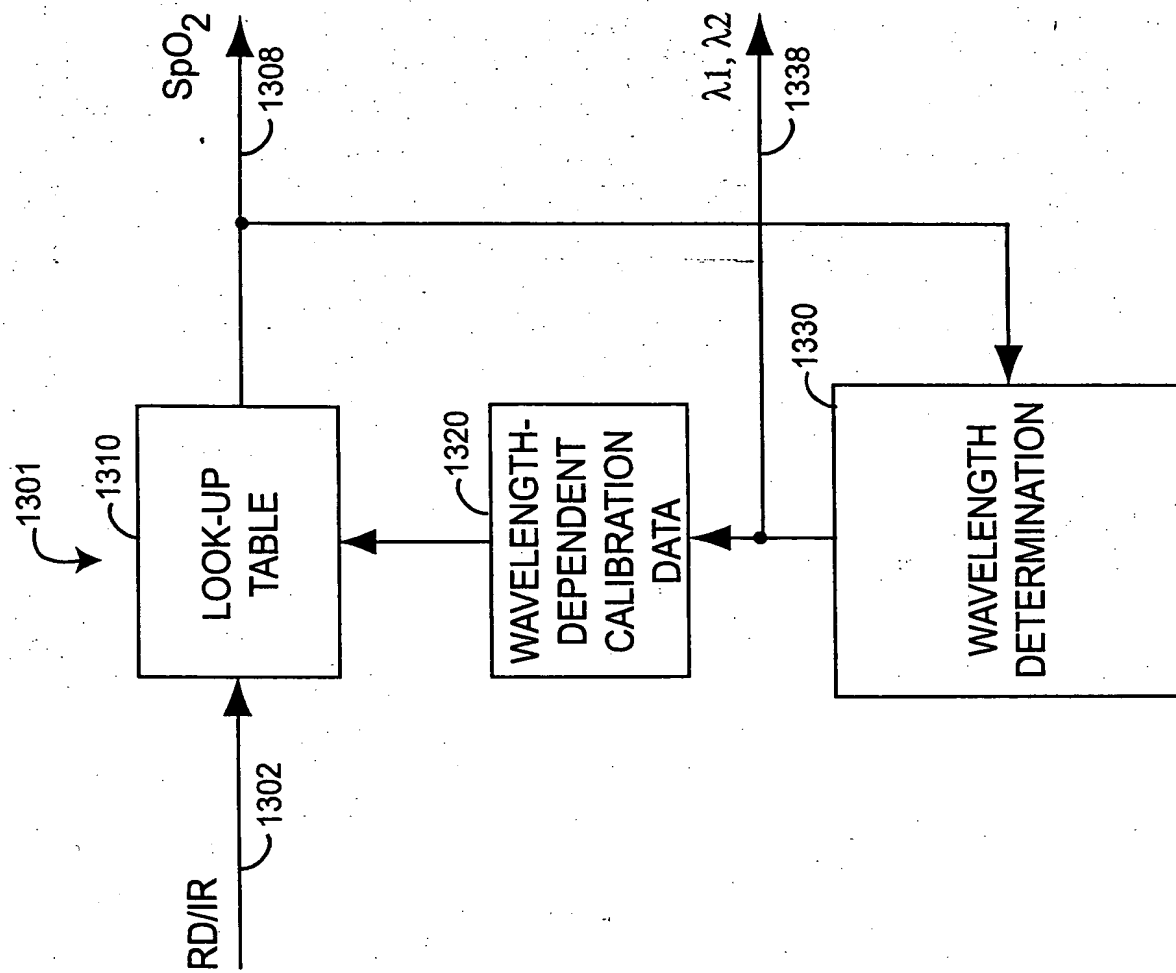


FIG. 13B

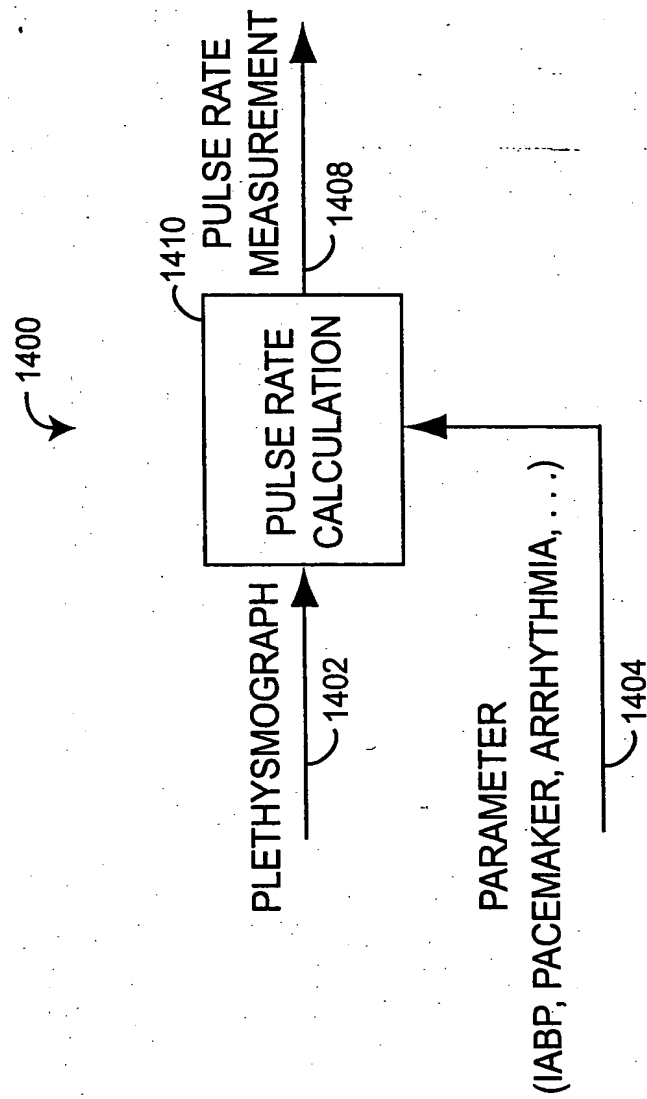


FIG. 14